

THE FOLLOWING PAGE CONTAINS THE CONNECTION DETAILS

It is your responsibility to ensure that the transducer identification matches the connection details, including any RDP modification (T.M) references.

Please ensure that the transducer has not been modified or fitted with a cable or extension.

Particularly on DC-DC powered transducers, incorrect connection may cause **IRREPERABLE DAMAGE** to the transducer which is **NOT COVERED BY WARRANTY**

IF YOU ARE IN ANY DOUBT PLEASE CONTACT US

DESPATCH:- INCLUDE CD1023 IF TRANSDUCER HAS NO CABLE FITTED.



DCW SERIES

(STD. O/P, CABLE OPTIONS 6 & 9)



CONNECTION DETAILS


Dual Supply
+10 to +20V Input
-10 to -20V Input
0V Common I/P, O/P
Output
Instrument Ground

WIRE/PIN
RED/1
BLUE/3
GREEN/4
YELLOW/2
SHIELD


Single Supply *
20 to 40V Input (Vs)
Supply Common
Output Common **
Output
Instrument Ground

* SUPPLY MUST BE FULLY FLOATING
 ** OUTPUT COMMON FLOATS AT Vs/2

WIRE/PIN
RED/1
BLUE/3
GREEN/4
YELLOW/2
SHIELD

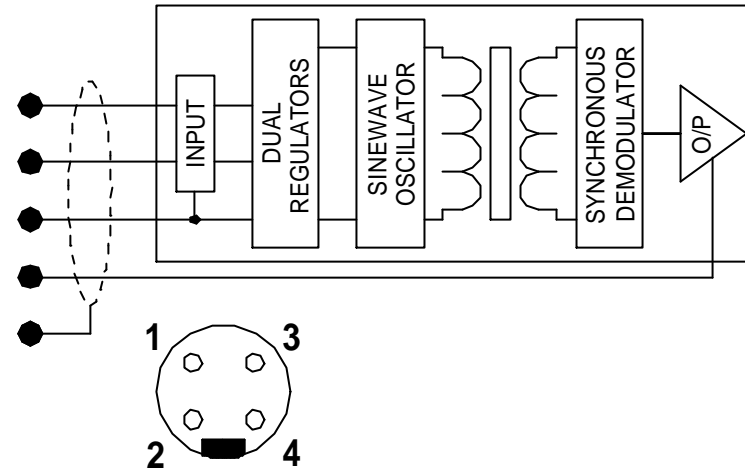

LOAD IMPEDANCE: 2k (min.) Ohms with dual supply.
 20k (min.) Ohms with single supply.
SUPPLY: Smooth d.c. voltage 25mA typical

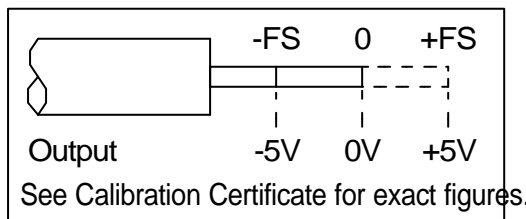

NOTE : INCORRECT CONNECTION MAY CAUSE IRREPARABLE DAMAGE
 CONTACT OUR SALES DEPARTMENT IF YOU REQUIRE ASSISTANCE
 For transducers without cable see CD1023 for fitting instructions.

RDP U.K.
 Tel 01902 457512
 Fax 01902 452000



Certificate No. FM 13141
 BS EN ISO 9001:2000

MADE IN THE
 UNITED KINGDOM

Doc. Ref. WDUK1456
 ISSUE 3 - 21 APR 2004

RDP U.S.A.
 Tel 610 469 0850
 Fax 610 469 0852

Distribuidor

Brasil e América do Sul

CONTATO

Endereço

Rua Sete de Setembro, 2656 - Centro
13560-181 - São Carlos - SP - Brasil

Telefone

+ 55 (16) 3371-0112
+ 55 (16) 3372-7800

Internet

www.metrolog.net
metrolog@metrolog.net

